



Installation Instructions Model MWLT200, Class 1 Series AC-DC Power Supply

AC INPUT : 100-240 VAC, 3.0 A
47-63 Hz

SAFETY APPROVALS: UL Recognized to UL60601-1
CAN/CSA C22.2 /IEC/EN60601-1 3rd Ed.

(Input selection is automatic; no manual change is required.)

DC OUTPUT:

Model Number	Output Connector	Voltage	Max. Load (Convection)	Max. Load (300 LFM)	Min. Load
LFMWLT200-1000	Screw Terminal	V1=5V	26.0A	35.0.0A	0.0A
LFMWLT200-1001	Screw Terminal	V1=12V	13.33A	16.67A	0.0A
LFMWLT200-1002	Screw Terminal	V1=15V	10.67A	13.33A	0.0A
LFMWLT200-1003	Screw Terminal	V1=24V	6.67A	8.33A	0.0A
LFMWLT200-1004	Screw Terminal	V1=48V	3.33A	4.17A	0.0A
LFMWLT200-1005	Screw Terminal	V1=30V	5.33A	6.67A	0.0A
LFMWLT200-1300	Header Type	V1=5V	26.0A	26.0A	0.0A
LFMWLT200-1301	Header Type	V1=12V	13.33A	16.67A	0.0A
LFMWLT200-1302	Header Type	V1=15V	10.67A	13.33A	0.0A
LFMWLT200-1303	Header Type	V1=24V	6.67A	8.33A	0.0A
LFMWLT200-1304	Header Type	V1=48V	3.33A	4.17A	0.0A
LFMWLT200-1305	Header Type	V1=30V	5.33A	6.67A	0.0A

– CAUTIONS & NOTES –

CAUTION: This component level power supply is intended exclusively for installation within other equipment by an industrial assembly operation or by professional installers. This is a Class I power supply; the unit must be properly connected to earth ground in end use. A component power supply should be installed in end-use equipment according to the requirements of the safety standard used for that equipment. This power supply is not designed to be operated outside of an enclosure which provides a means of mechanical, electrical, and fire protection. To maintain SELV requirements, the outputs should not be connected together in any manner which causes the total output voltage to exceed 60 VDC.

WARNING: This is a Class A product. In a domestic environment this product may cause radio interference in which case the user may be required to take adequate measures.

PROTECTIVE EARTHING:

The Power Supply must be properly grounded to mains protective earthing termination at end use.

ENVIRONMENTAL CONDITIONS:

Transportation & Storage

Ambient Temperature Range: -40 °C to +70 °C
Relative Humidity Range:
5 % to 95 % RH Non-Condensing
Altitude: 40,000 ASL Feet

Operation

Ambient Temperature Range: 0 °C to +50 °C
Relative Humidity Range:
5 % to 95 % RH Non-Condensing
Altitude: 10,000 ASL Feet

Additional application information is available from the EOS web site at www.eospower.com

EOS Power India Pvt. Ltd.
Unit # 57, SDF II, SEEPZ, Andheri (East); Mumbai 400 096, India
Phone: +91 22 67744000



Installation Instructions Model MWLT200, Class 1 Series AC-DC Power Supply

FUSING and SERVICING:

Fuse is F1 & F2, rated F 5 A, 250 V. In case of failure, the Power Supply must be returned to EOS Power Authorized Service Center. There are no user-serviceable parts in the Power Supply.

LIMITED WARRANTY:

EOS Power warrants each power supply of its manufacture for a period of two years from the date of manufacturing. This warranty applies to defects in materials and workmanship that result in non-performance to published specifications.

EOS Power assumes no liabilities for consequential damages of any kind through the use or misuse of its products by any user. No other obligations are expressed or implied.

Please note that the specifications, terms, and conditions stated are subject to change without notice.


NUCLEAR AND MEDICAL APPLICATIONS:

EOS Power products are not designed, intended for use in, or authorized for use as critical components in life support systems, equipment used in hazardous environments, or nuclear control systems without the express written consent of the respective divisional president of EOS Power, Inc.

TECHNICAL REVISIONS:

The appearance of products, including safety agency certifications pictured on labels, may change depending on the date manufactured. Specifications are subject to change without notice.

MECHANICAL DIMENSION:

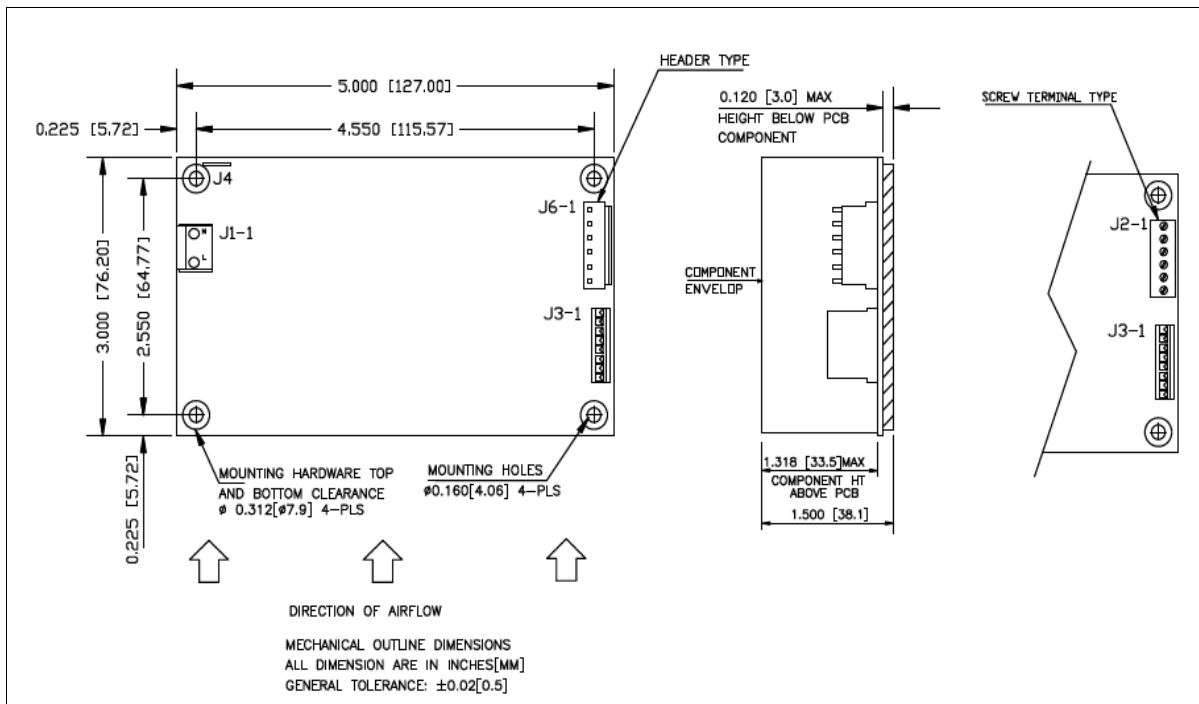

Additional application information is available from the EOS web site at www.eospower.com

EOS Power India Pvt. Ltd.
Unit # 57, SDF II, SEEPZ, Andheri (East); Mumbai 400 096, India
Phone: +91 22 67744000



Installation Instructions Model MWLT200, Class 1 Series AC-DC Power Supply

PIN ALLOCATION :

Pin	Name	Description
Input J1 & J4		
J1-1	Neutral	AC Input Neutral
J1-2	Line	AC Input Line
J4	Earth	AC Input Earth
Output J2		
Pin 1-2-3	GND	Output return
Pin 4-5-6	V1	V1 Main output
Signal J3		
J3-1	V1 Sense +	Main output V1 positive sense
J3-2	V Fan	Fan output voltage (+12V/0.5A)
J3-3	V1 Sense -	Main output V1 negative sense
J3-4	Remote ON/OFF	Remote ON/OFF
J3-5	V stby	Standby output voltage (+5V/1A)
J3-6	GND	Output return for signal
J3-7	Power Fail	Power fail signal for V1
J3-8	Power good	Power good signal for V1

Connector Mating Parts (Molex or equivalent) :

CONNECTOR	HOUSING	CRIMP TERMINAL	WIRE GAUGE
J1	09-50-3031	08-50-0106	AWG # 18
J4	190030001	-	AWG # 18
J2 (Screw Terminal)	-	-	AWG # 13
J6 (Header Type)	VHR-6M	SVH-41T-P1.1	AWG # 18
J3	22-01-2087	08-50-0113	AWG # 24

Additional application information is available from the EOS web site at www.eospower.com

EOS Power India Pvt. Ltd.
Unit # 57, SDF II, SEEPZ, Andheri (East); Mumbai 400 096, India
Phone: +91 22 67744000